Medtronic Custompack Specifications

Hospital	Erasmus MC	Chief Perfusionist	Dwight Dumay
City	Rotterdam	Sales–Representative	Tim Teunissen
Country	Nederland		

Rev	Date	Draftsman Init	Draftsman Signed	Remarks
A	29.11.2023	F.E.		New Drawing (based on M310933C)
B	11.12.2023	F.E.		change item 8, 10, 11, 12 & purge line
C	07.11.2025	M.C.		Changes in entire drawing
D	01.12.2025	M.C.		Remove AP40
E	19.12.2025	F.E.		Remove lines

PACKAGING INFORMATION CLEANROOM		NR
Tray	: Midi Tray	1.00
Lid	: Tyvek Cover	1.00
Bag	:	
Label	: End–label	1.00


PACKAGING INFO PACKAGING DEPARTMENT		NR
U–Box	: 76x21x41 cm	1.00
M–Box	: 1 SETS IN 1 BOX	
Inserts	: Midibox insert	1.00
Label	: End–label	1.00
	IFU Custom pack	1.00

DRAWING IS ACCORDING PROC. PE 2004
REF. TO ALL APPLICABLE CLEANROOM PROC.
AND Q.A. REQUIREMENTS
ALL PACKS STERILIZED PER CYCLE 79

Sterilisation load : 0.095 m3

NOTE:
PUT WRAP 30x30" ON TOP

Midi Tray

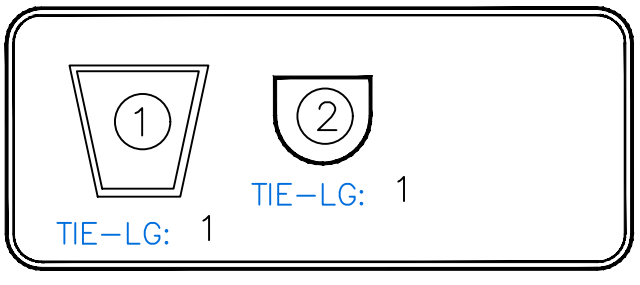


1 FUSION CVR FLAT
2 FUSION OXY

APPROVAL	SIGNED	DATE
ENGINEERING		
MANUFACTURING		
QUALITY ASSURANCE		

Pack Title : BB ADULT OPEN FUSION SET 1/B
Att.refcode : 161100110101101

DRAWING NUMBER
M310936E

Medtronic Custompack Specifications

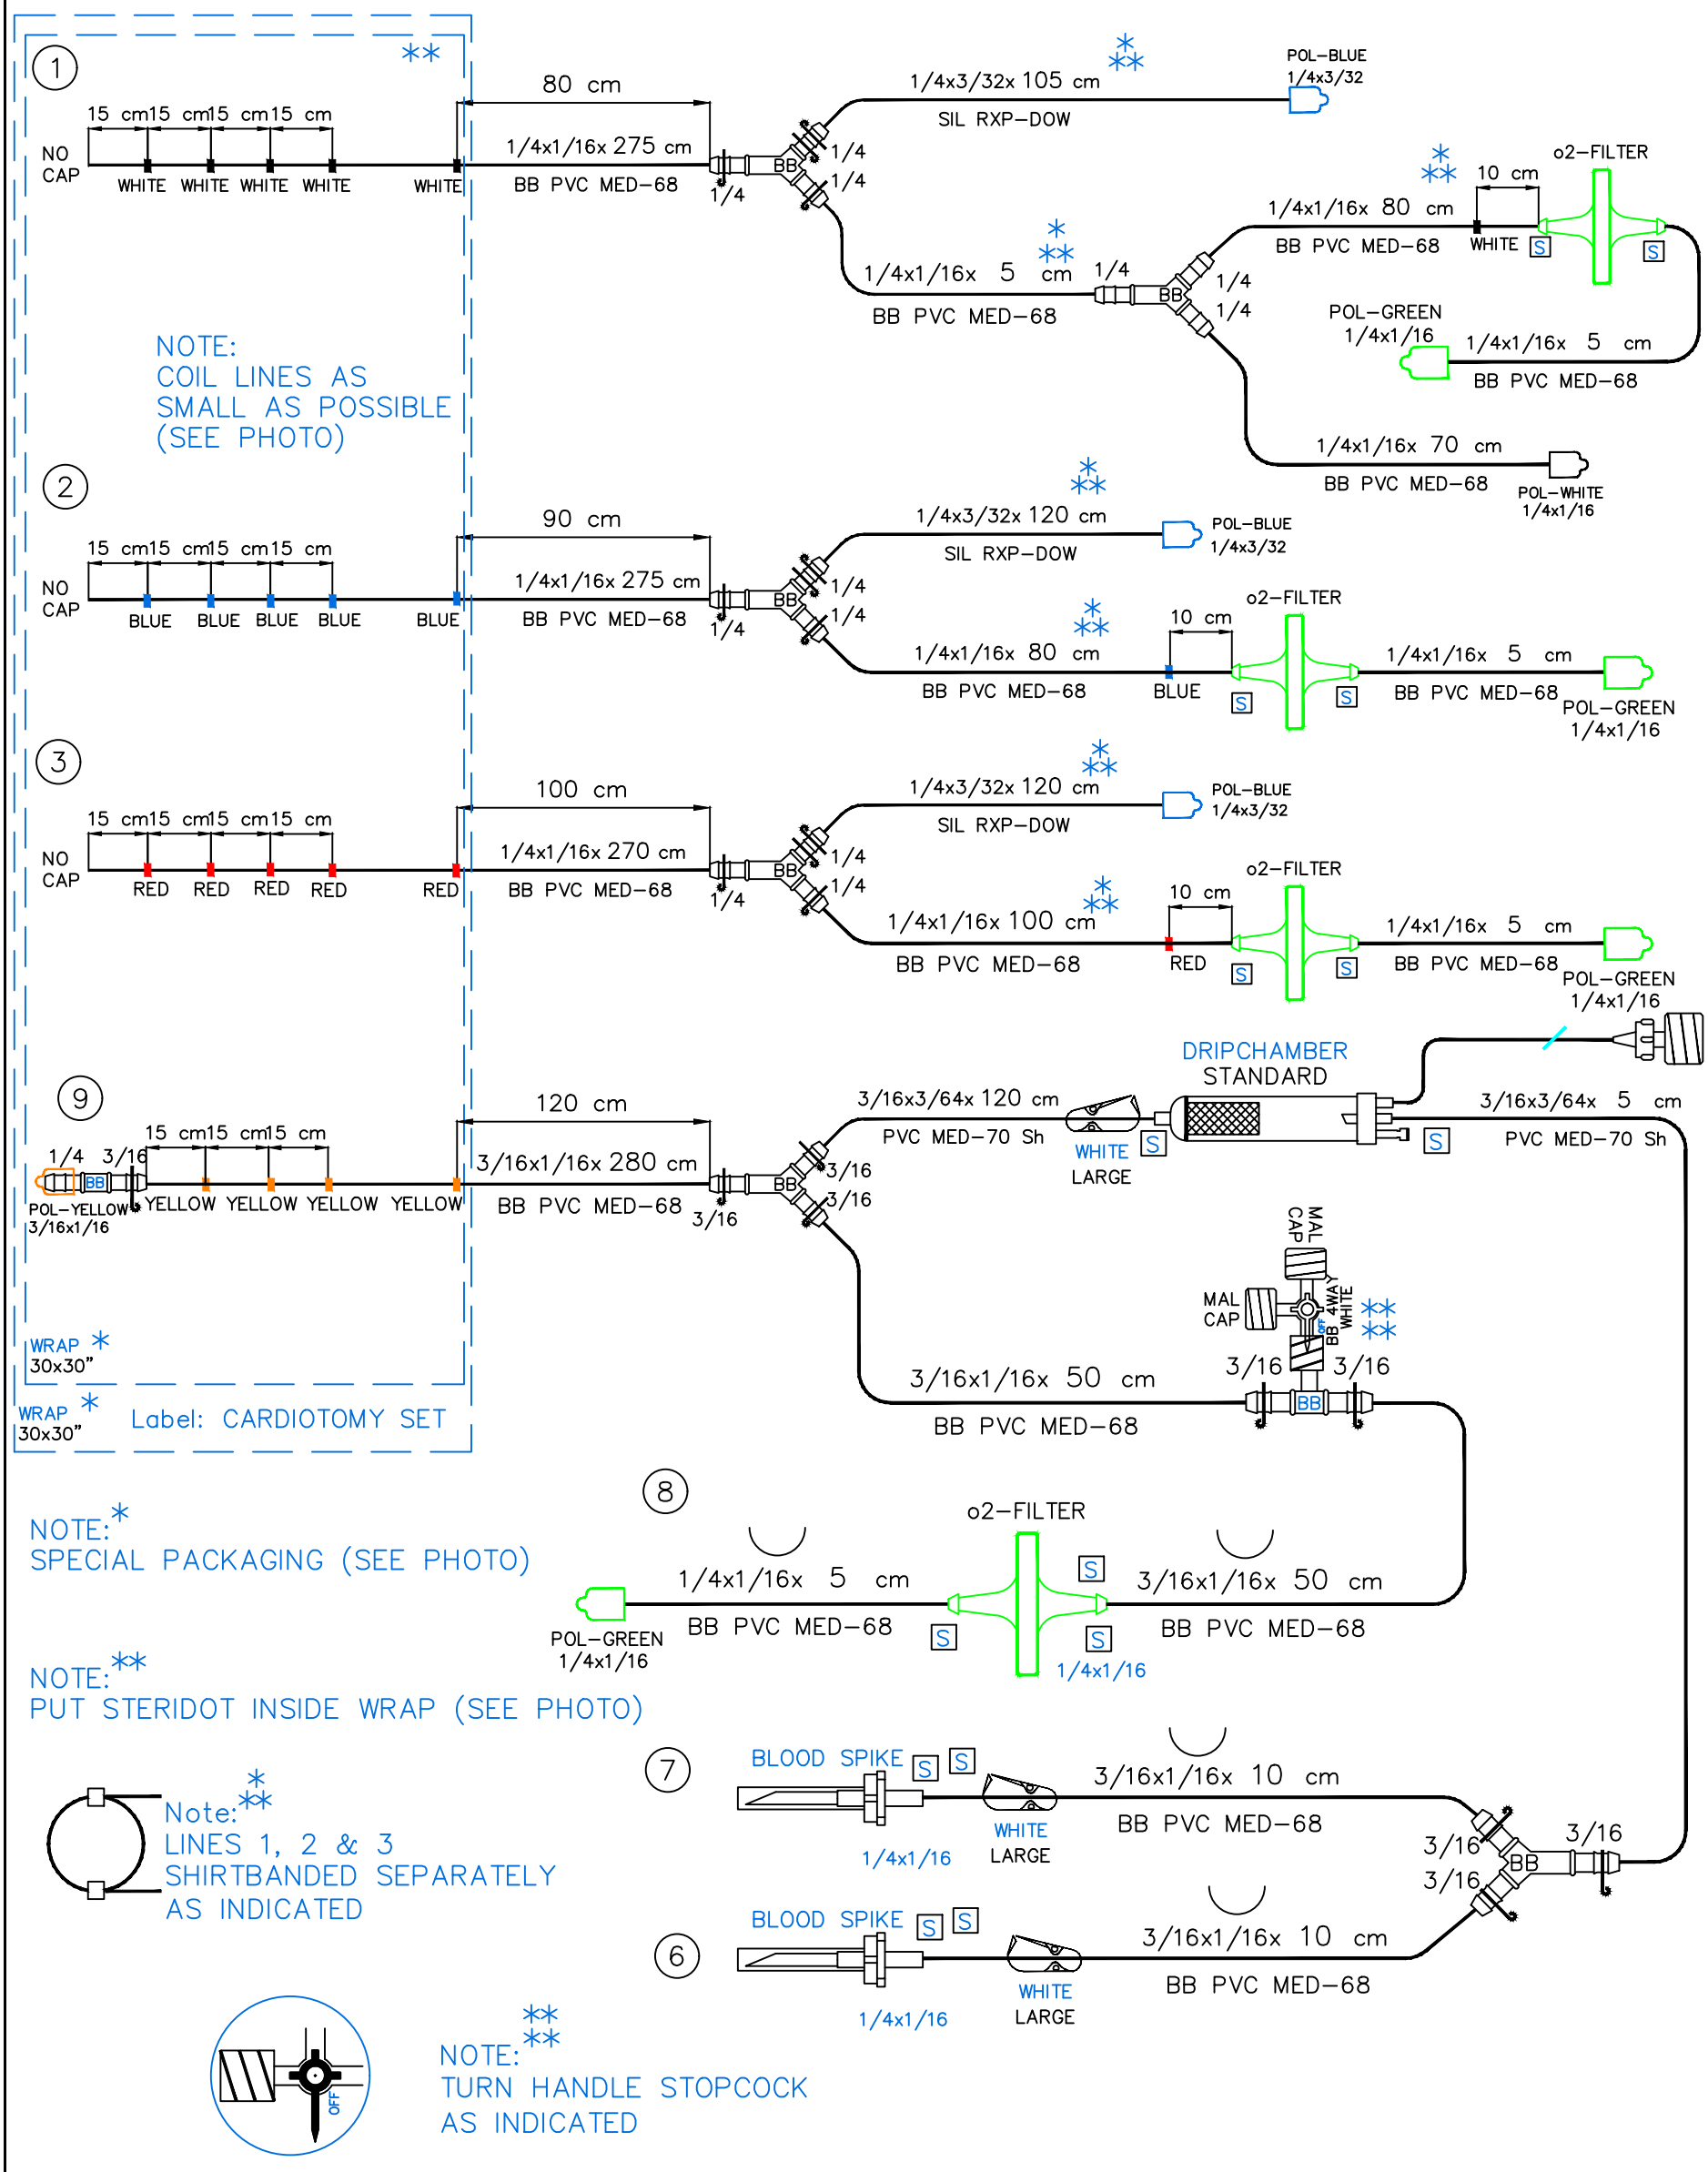


Pack Title : BB ADULT OPEN FUSION SET 1/B


Att.refcode : 161100110101101

DRAWING NUMBER

M310936E

Medtronic Custompack Specifications

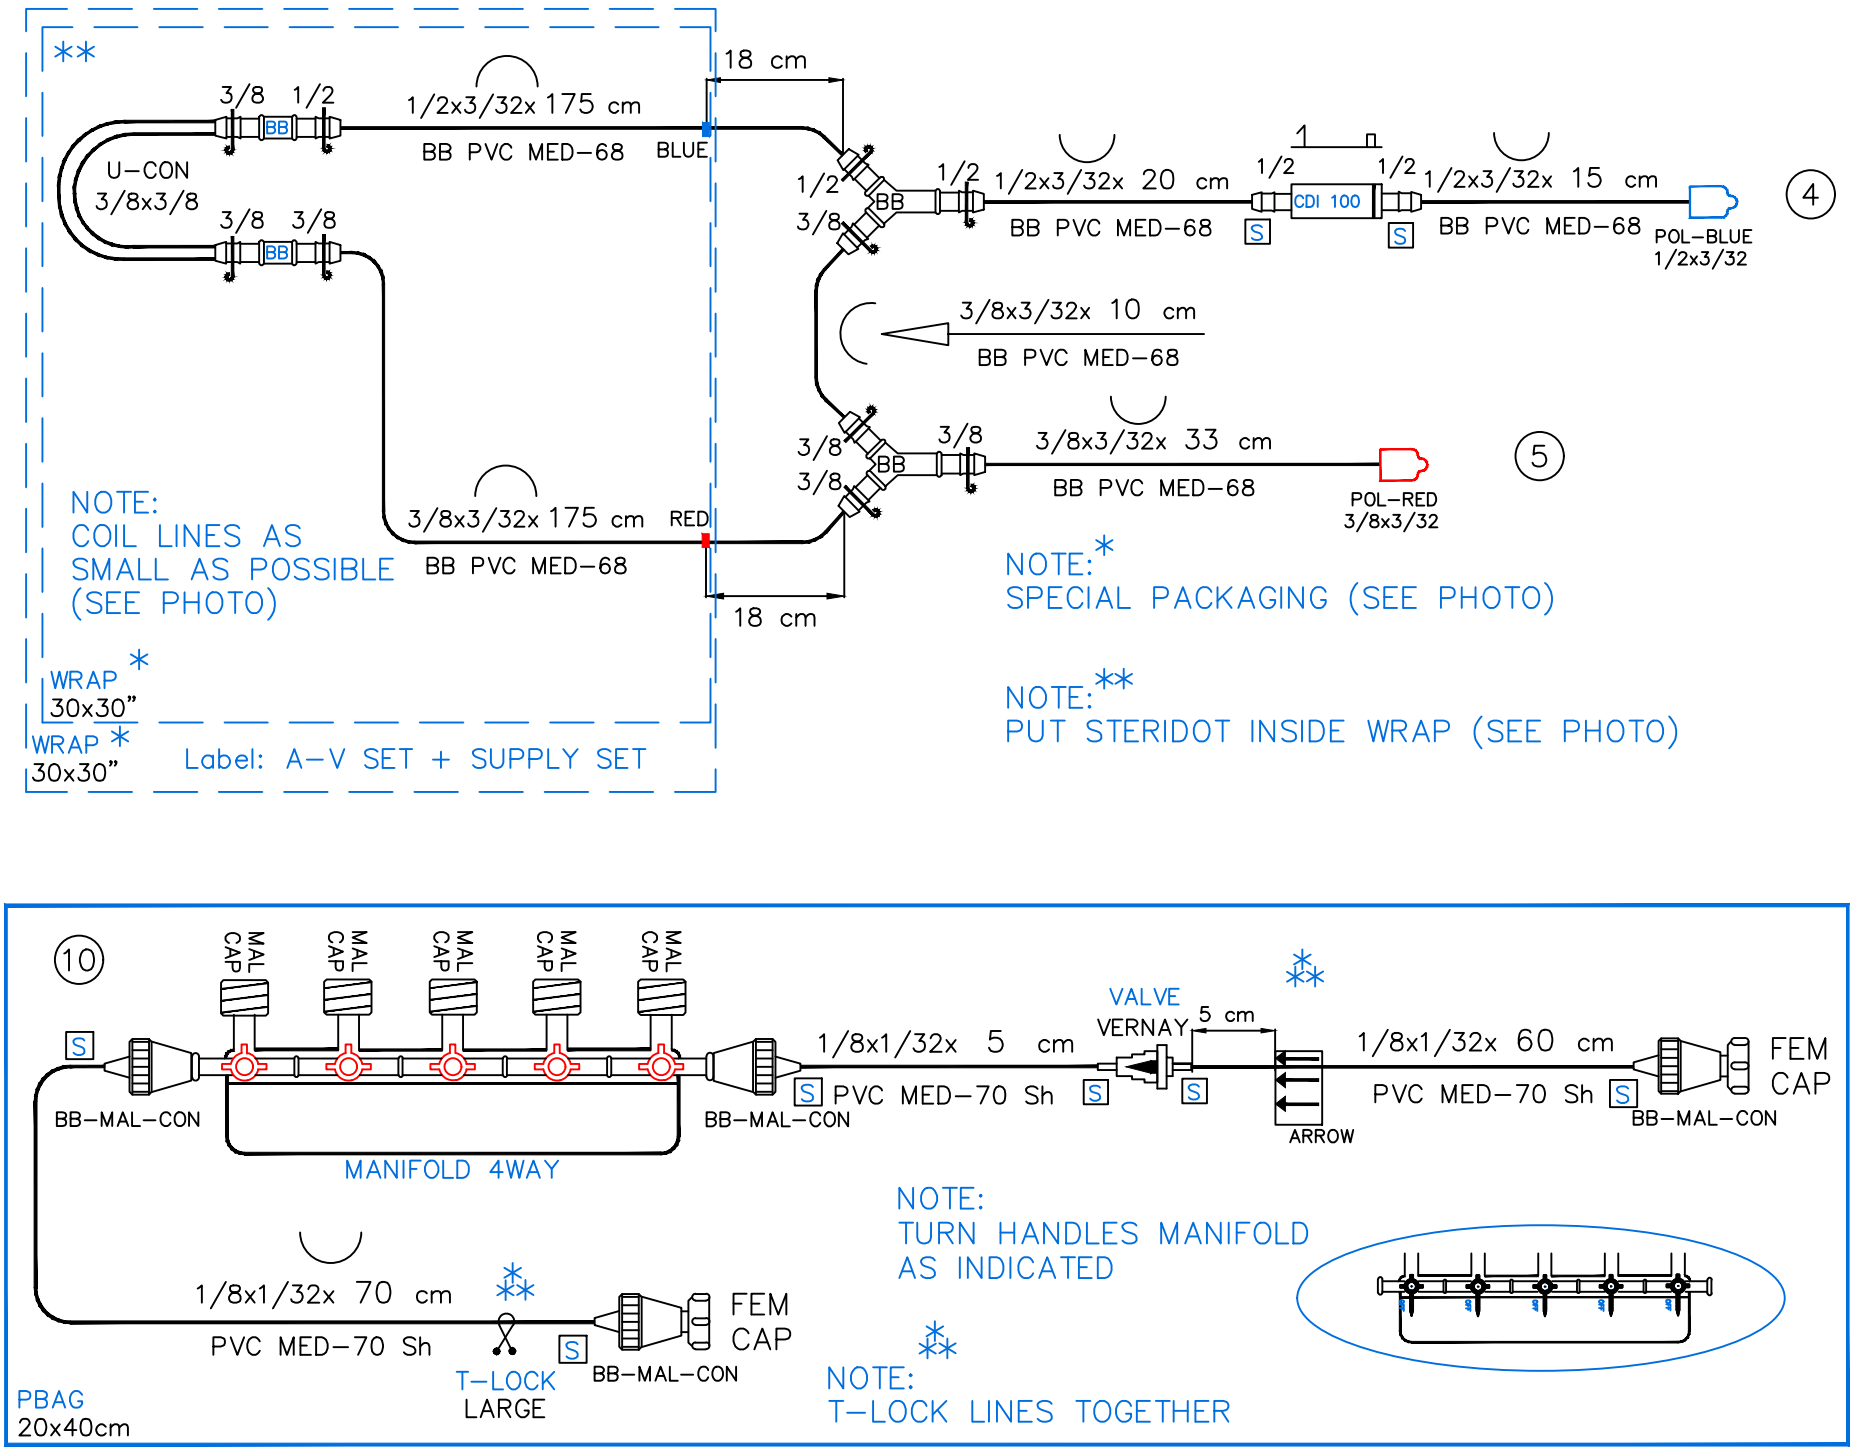

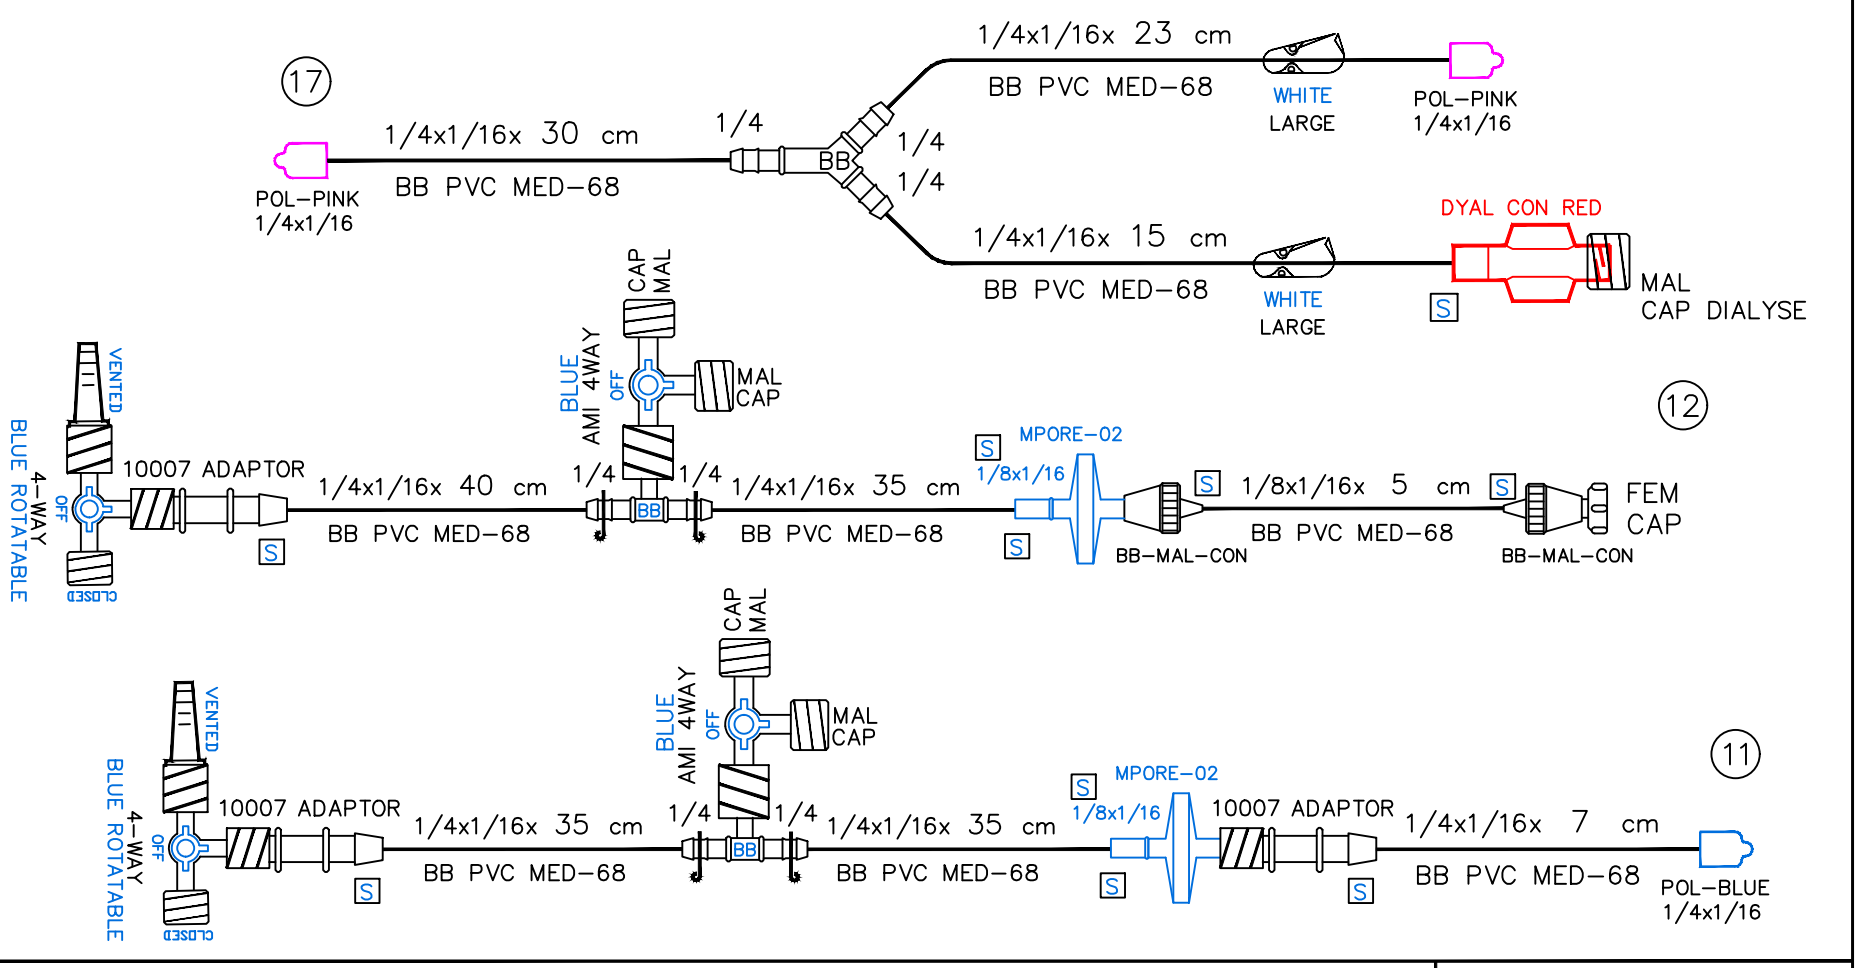


Pack Title : BB ADULT OPEN FUSION SET 1/B

Att.refcode : 161100110101101

DRAWING NUMBER

M310936E

Medtronic Custompack Specifications

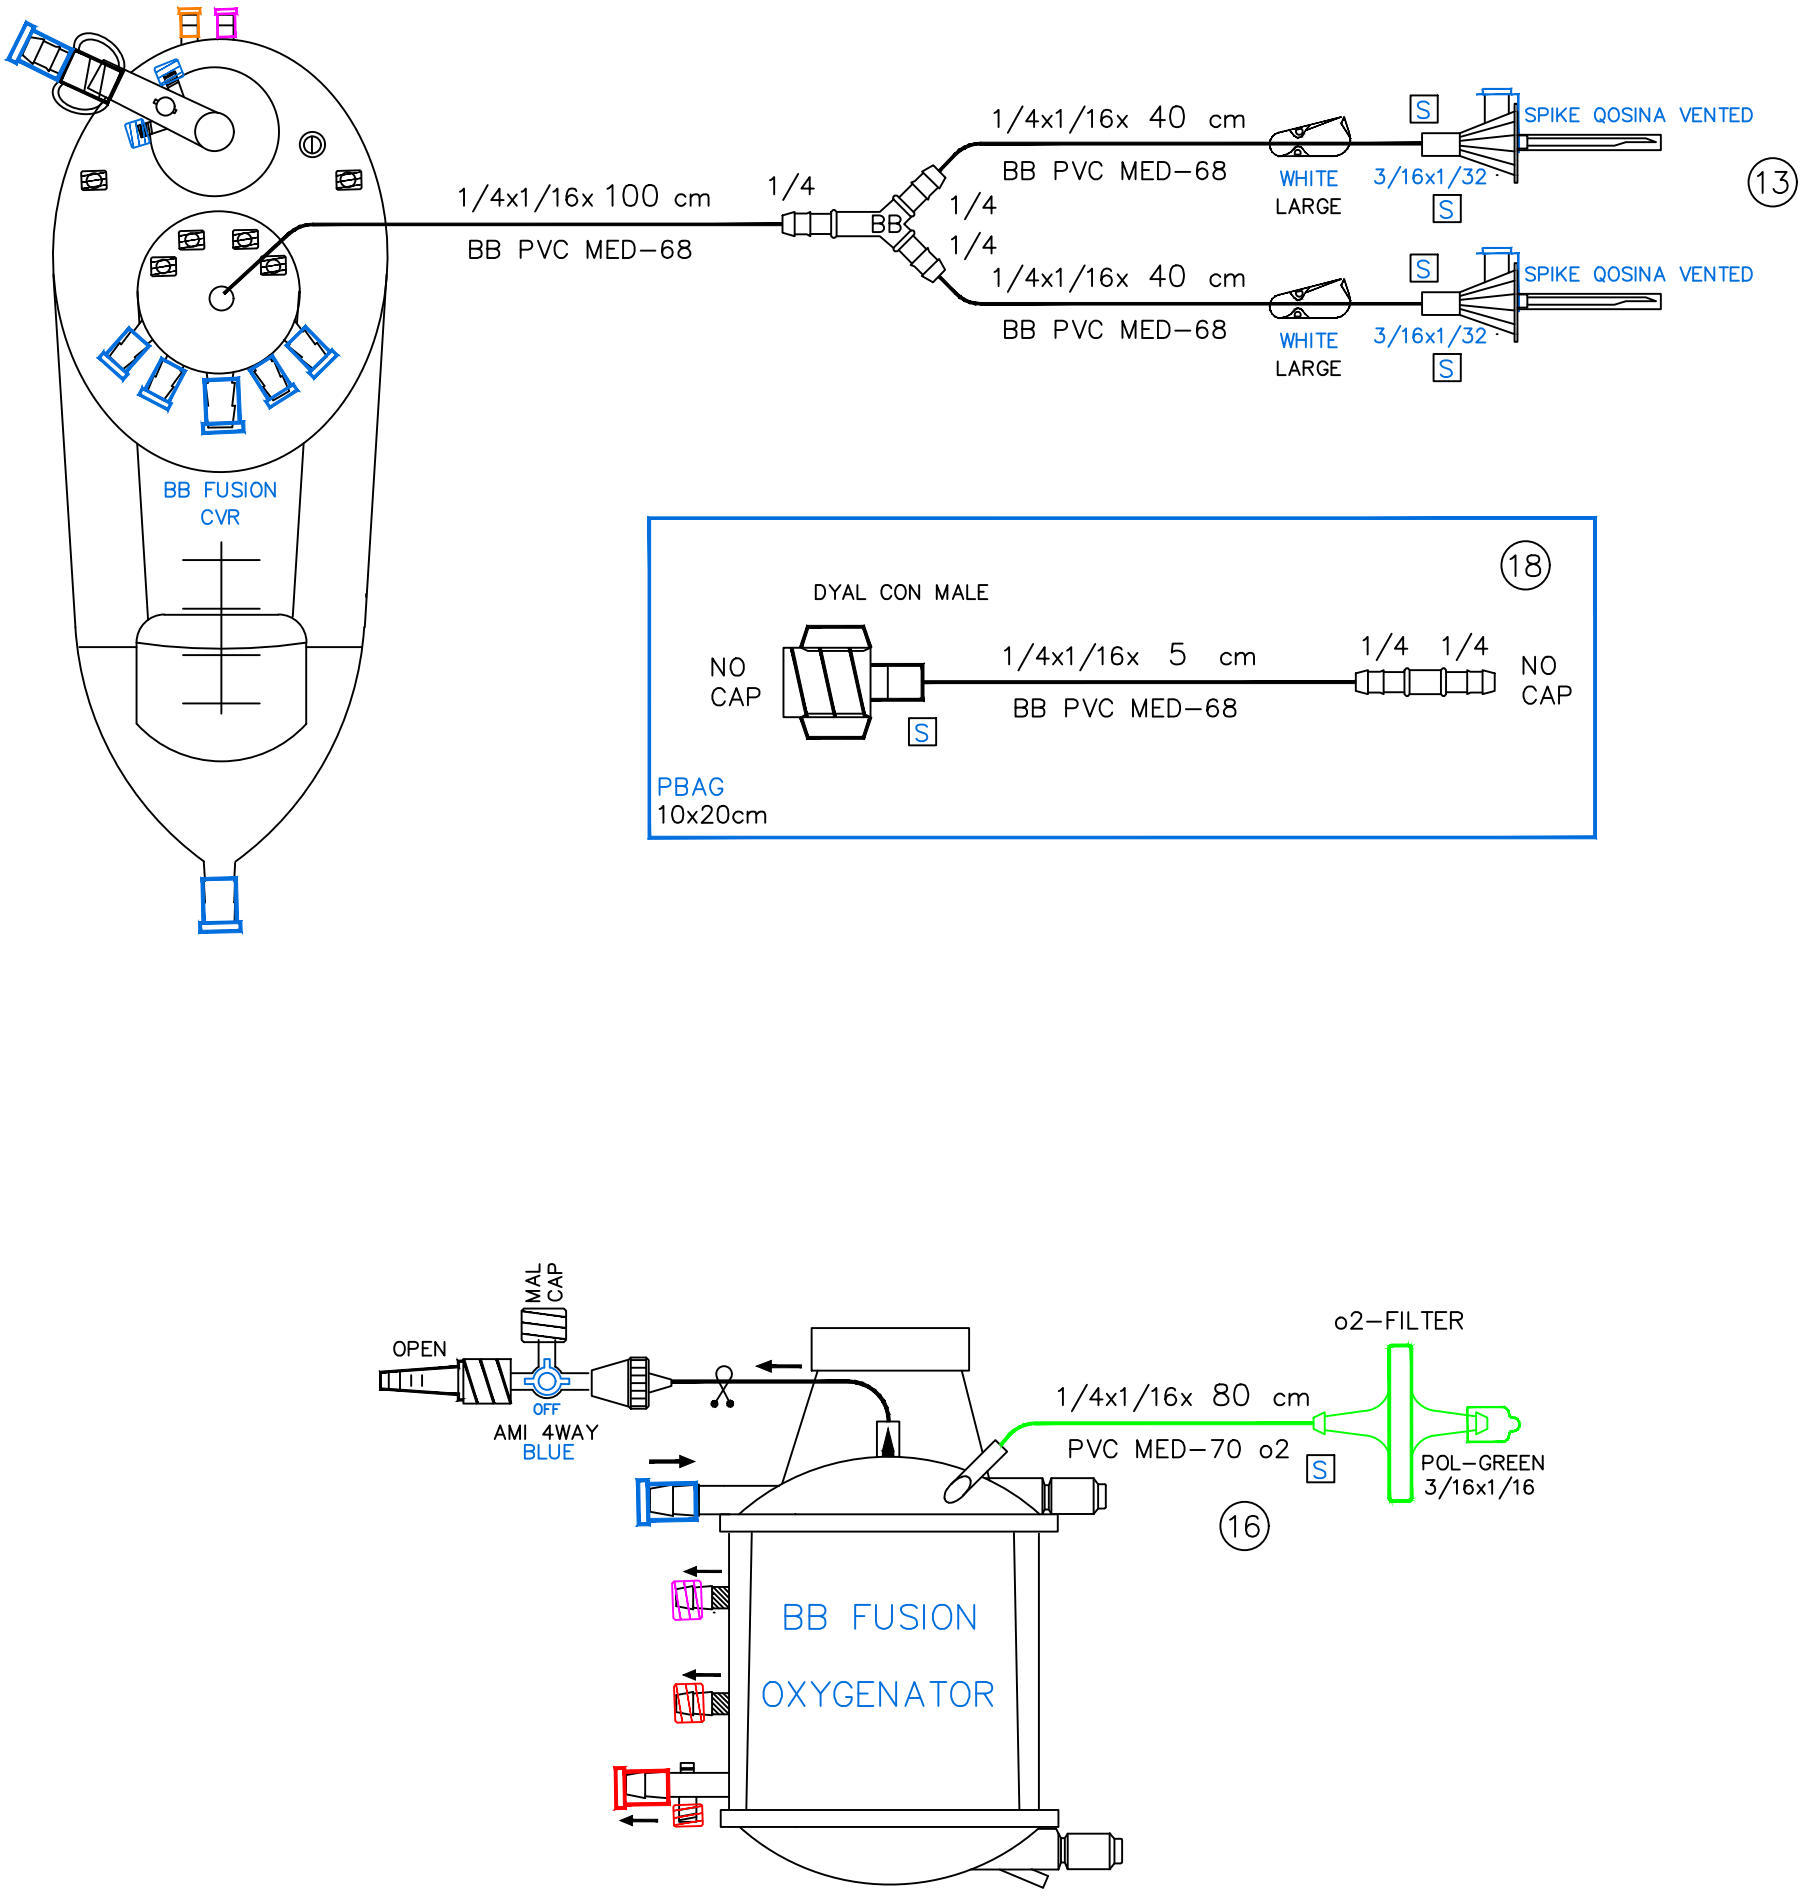

Pack Title : BB ADULT OPEN FUSION SET 1/B	DRAWING NUMBER
Att.refcode : 161100110101101	M310936E
Page 4 Of 4	